



UV/NIR - 3700 UV-Visible/NIR Spectrophotometer



EPCC / PRODUCTS / APPLICATION / SOFTWARE / ACCESSORIES / CONSUMABLES / SERVICES

Analytical Technologies Limited

An ISO 9001 Certified Company

www.analyticalgroup.net



Features

Continuously Variable Slit

Through the use of a continuously variable slit, low-noise measurements can be made over a broad wavelength region including the ultraviolet, visible, and near infrared (190 to 3,300 nm)

Low Stray Light, High Photometric Range

Achieves best-in-class levels of low stray light and high photometric range through use of a Czerny-Turner mounted single-monochromator bright spectrometer and a newly-developed grating*1

Supports high-speed scanning

Employs a gear-drive system to realize high-speed scanning of the visible, ultraviolet, and near-in-frared regions

Supports high-speed scanning

Employs a gear-drive system to realize high-speed scanning of the visible, ultraviolet, and near-in-frared regions

New control and data-processing software

A more comfortable operating environment using UV Solutions Plus

Many accessories

A line-up of accessories to support a wide range of measurement objectives


Hardware


Handling the ultraviolet, visible, and near-infrared regions (190 to 3,300 nm), the UV/NIR 3700 achieves both high measurement precision and high throughput



>> Use of a continuously variable slit


The UV/NIR 3700 employs a continuously variable slit in the near-infrared region, in which the slit automatically widens when measuring low quantities of light and narrows when measuring large quantities of light, and thereby achieves low-noise measurements across a broad range of measurement wavelengths from 190 to 3,300 nm.

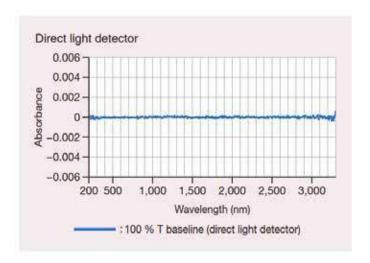


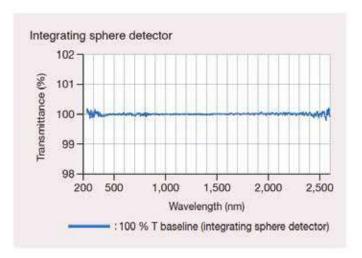

Low stray light

The UV/NIR 3700 achieves best-in-class levels of low stray light and high photometric range through use of a Czerny-Turner mounted single-monochromator bright spectrometer and a newly developed grating using photolithography technology.*2

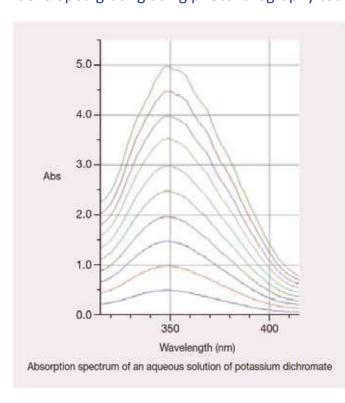


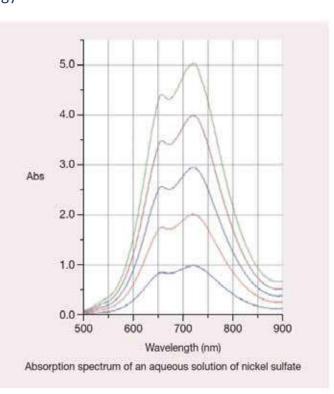



Measurement throughput improvements

By employing a gear-drive system for the wavelength drive, high scanning speeds compared to conventional instruments are achieved of approximately 0.3 to 5,000 nm/min in the ultraviolet-visible region.*3 When measuring at a 1 nm interval, a measurement made at 1,000 nm/min in the 190 to 3,300 range can be completed in approximately 4 minutes.

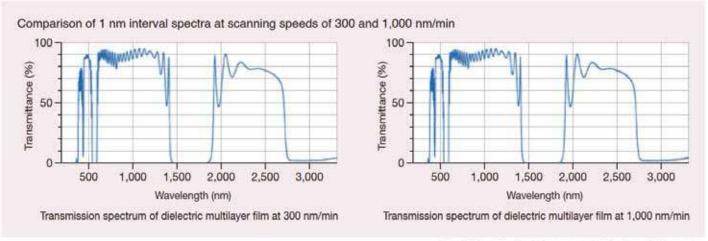


*3 U-3900 : 1.5 to 2,400 nm/min, U-2900 : 10 to 3,600 nm/min,

Control of detector switching level difference

Generally, UV/NIR 3700/near-infrared spectrophotometers use different detectors in the UV-visible region and the near-infrared region. Because different detectors are used, a difference in photometric values may arise in switching between detectors. Through know-how developed from the fundamentals, signal processing technology, and other techniques, the UV/NIR 3700 holds the level difference when switching detectors to a minimum.

Example of a measurement near the detector switching wavelength (absorption spectrum of an infrared light absorbing material)

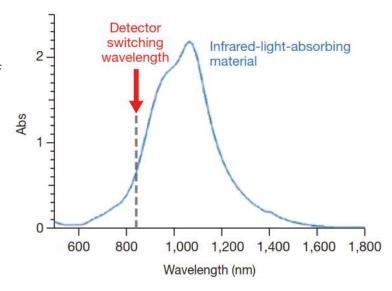



>> Common utilization of accessories

The sample compartment shares a common design with the spectrophotometers, so you can use the accessories you already have.*4 We offer an extensive line-up of accessory types tailored to measurement objectives.


*4 Except for certain accessories (please check with your sales representative for details)

Software

Simple operation flow and abundant data processing features make analysis pleasant

>> Use of new control and data processing software UV Solutions Plus

Enhancements have been added compared to the popular UV Solutions including a tabular form display feature for data lists and data processing results, a report layout feature, a performance confirmation feature, and more.

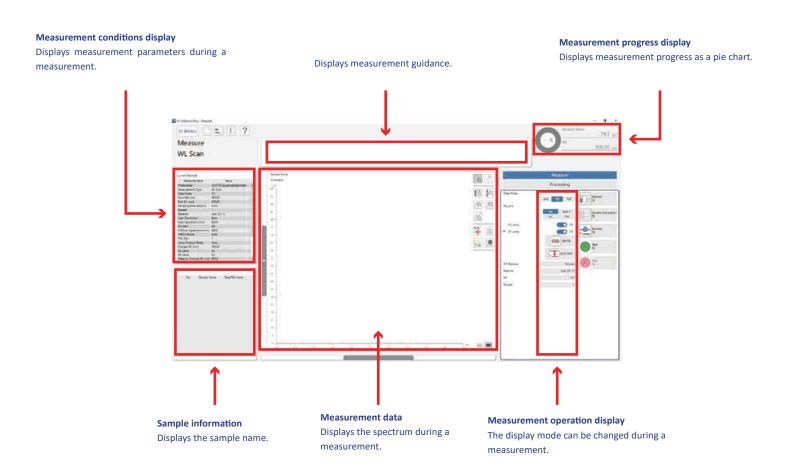



>> Operation flow

The measurement operation buttons are located on the right side. A measurement can be made using basic operations in four steps.



1 Set Analysis Conditions

Press Analysis Conditions and set the conditions.

2. Set Sample Information

Detailed conditions related to the measurement sample, the storage location for data, and other parameters can be set.

3. Baseline

Perform baseline correction.

4. Measurement Start

Start the measurement.


>> Many added features that follow in the footsteps of existing operability

- Change the wavelength unit of a monitored value during measurement
- Measurement progress display
- Photometric value unit conversion (Abs, %T, %R, etc.)
- Direct display of the concentration calculated from coefficients
- Batch data processing of multiple files, and more

Measurement progress display





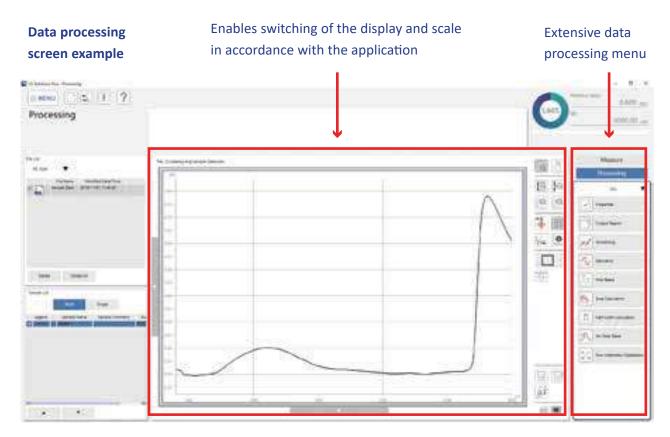

>> List display feature for data processing results

Specific wavelength data, area calculation data, half-value width calculation data and other data across multiple samples can be displayed in tabular form. Comparing data between samples can be done easily. In addition, you can return to raw data after storing processed data.

Reporting function

More effective for preparing reports.

You can freely lay out printable items such as analysis conditions, data processing results, spectra, etc. with the report layout feature, which did not exist in the UV Solutions software in the past. You can also print designated image data (jpg, png, and bmp).


>> Standard installation of performance confirmation feature

This feature can check for proper function and performance on a daily basis.

Performance confirmation feature items: wavelength accuracy, wavelength setting repeatability, noise level (RMS), baseline flatness, baseline stability, spectral band width, photometric accuracy, stray light, group editing of performance confirmation items, graphical display of performance confirmation results history.





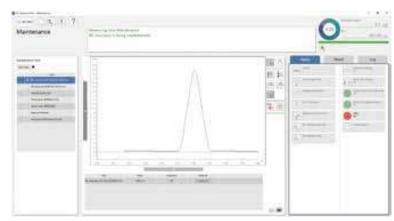



Application

Supports problem solving for a variety of applications

Measurement of hexavalent chromium (diphenylcarbazide absorptiometry)

We present an example of analysis by diphenylcarbazide absorptiometry of hexavalent chromium, which is subject to regulation by the RoHS directive. Hexavalent chromium was measured using "Reagent Set for Water Analyzer No. 31 Chromium (Hexavalent)" Chemical-Check Lab., Corp. From the absorption spectrum measurement results, the presence of an absorption peak at a wavelength of 540 nm was confirmed. Good linearity was obtained for the calibration curve at the 540 nm absorption peak with $R^2 = 1.0000$.

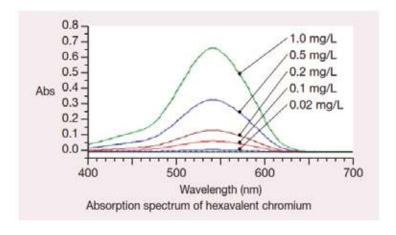

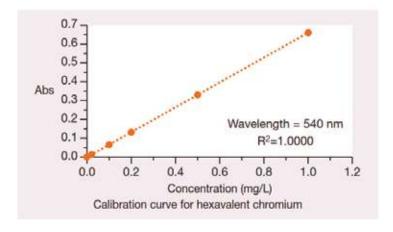





Measurement of silica (molybdenum yellow absorptiometry)


The measurement for silica by molybdenum yellow absorptiometry is prescribed in JIS K0101 Testing Methods for Industrial Water. Silica was measured using "Reagent Set for Water Analyzer Silica". From the absorption spectrum measurement results, the presence of an absorption peak at a wavelength of 815 nm was confirmed. Good linearity was obtained for the calibration curve at the 815 nm absorption peak with R²


= 0.9999.

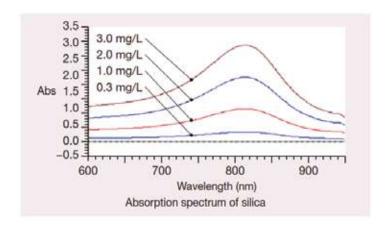

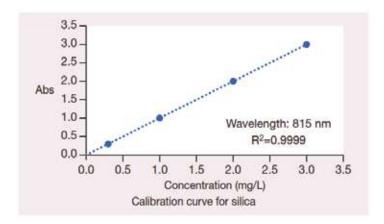

Color measurement (optional package)







Color calculation results


Reflection spectra and chromaticity coordinates of cosmetic products


The light source, field of view, and other such parameters were set using spectra from the standard method (wavelength range 360 to 830 nm, 1 nm interval) and the practical method (wavelength range 380 to 780 nm, 5 nm interval), and color calculations were carried out. Color calculation results can be plotted onto chromaticity coordinates.



Measurement of filters


Filters allow light at specific wavelengths to pass through. Filters A, B, and C passed light in the blue, green, and red regions, respectively, and filter D passed light in the entire visible region.

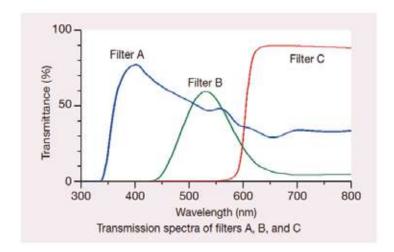


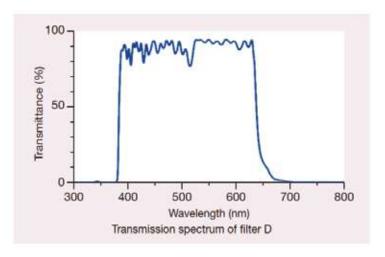

Measurement of window glass and coatings


Near-infrared light from the sun is a source of heat that can pass through glass windows and cause the temperature of a room to rise. Because of this, functional glass has been employed in recent years that cuts near-infrared light. In addition, functional coatings have been used on the outer walls of buildings to reflect near-infrared light. The optical characteristics of functional glass and functional coatings were measured.

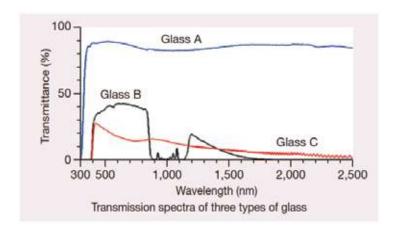

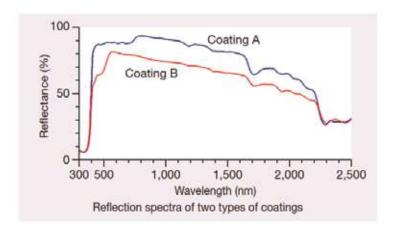



Calculations using optional package



Light/solar direct (glass) calculation results

Calculations can be performed that conform to the test methods pertaining to the transmittance (reflectance) of plate glass (visible light transmittance, solar transmittance, solar reflectance) as specified in Industrial Standards JIS R3106-2019.

| Data List Solar Reflectance Plant | | | | |
|-------------------------------------|-------------|-----------------|------------------------------|----------------|
| Nα. | Sample Name | Brightness (L*) | Solar Reflectance (ptr.) (%) | Judgment (psk) |
| 1 | Paint A | 95.33 | 84.83 | OK |
| 2 | Paint B | 90.16 | 69.79 | NG |

Solar reflectance (paint) calculation results

Calculations can be performed that conform to the method for obtaining the solar reflectance of paint specified in Industrial Standard JIS K5602-2008, and to the test method pertaining to high solar reflectance paint for roof use (solar reflectance) specified in Industrial Standard JIS K5675-2011.

Accessories

Accessory line up to support a broad range of measurements

The sample compartment shares a common design with the U-2900/U-3900, so existing accessories can be used.*5

*5 Except for certain accessories (please check with your sales representative for details)

Micro cell option

Micro cells are used in combination with a mask (2001537). A micro cell is suitable for small samples with volumes of 340 to 600 μ L.





| Product name | P/N | Capacity (μL) | Opticalpath length |
|-------------------------------|----------|---------------------|-----------------------|
| 10 mm micro quartz cell | 124-0357 | 340 ∼ 600 μL | 10 mm |
| Black 10 mm micro quartz cell | 200-0551 | 340 - 000 μΕ | 10111111 |
| Mask for micro cell | 200-1537 | _ | _ |



Ultra-micro volume sample measurement option

Trace sample cells are used in combination with a mask (3J1-0116) (2 included). These are suitable for ultra-micro volume with volumes of 1.5 to 90 μ L.



| Product name | P/N | Capacity (μL) | Opticalpath length |
|----------------------------|----------|---------------|-----------------------|
| 1.5 μL trace sample cell | 3J2-0120 | 1.5 to 4.0 μL | 1 mm |
| 12 μL trace sample cell | 3J2-0121 | 12 to 40 μL | 5 mm |
| 50 μL trace sample cell | 3J2-0122 | 50 to 90 μL | 10 mm |
| Mask for trace sample cell | 3J1-0116 | _ | _ |

Rectangular long-path cell holder (P/N 210-2107)

This holder is used when using rectangular long-path cells. Low-concentration samples can be measured with a high degree of sensitivity.



| Optical path length 10, 20, | , 30, 40, 50, 100 mm |
|-----------------------------|----------------------|
|-----------------------------|----------------------|

Water-circulating cell holder (P/N 210-2111)

Water from a thermostatic circulating water bath is circulated in the cell holder, and the cell section is kept at a constant temperature. (Temperature control: both R and S)



| Operating temperature range | Room temperature to 40°C |
|-----------------------------|--------------------------|
| Temperaturestability | Within ±0.3°C |

^{*}A thermostatic circulating water bath and front panel (P/N: 2J3-0182) are separately required when using this product .



Thermostatic cell holder with stirrer (P/N 2J3-0161)

A magnetic stirrer agitates the sample solution to limit the effect of temperature variation.

| Available cells | | Capacity |
|---|---------------------------|---------------|
| 10 mm rectangular cell | | 2.4 to 3.5 mL |
| Magnetic stirring cell made by Starna, Ltd. | 9-Q-10-MS, 29-Q-10-MS | 1.0 to 1.5 mL |
| | 18-Q-10-MS, 28-Q-10-MS | 600 to 800 µL |

^{*}A thermostatic circulating water bath and front panel (P/N: 2J3-0182) are separately required when using this product.

Programmable thermostatic cell holder (P/N 131-0301, 131-0302)

In protein and nucleic acid melting measurements, the sample temperature can be changed continuously to determine the variation in absorbance. Because it is heated and cooled electronically, this cell holder is capable of rapid heating and cooling. The sample temperature can be increased and decreased isothermally, and because this holder is equipped with a stirrer, there is no temperature variation within the cell. (temperature control: both R and S)In protein and nucleic acid melting measurements, the sample temperature can be changed continuously to determine the variation in absorbance. Because it is heated and cooled electronically, this cell holder is capable of rapid heating and cooling. The sample temperature can be increased and decreased isothermally, and because this holder is equipped with a stirrer, there is no temperature variation within the cell. (temperature control: both R and S)



| Usable cells | 10 mm cell (cell not included) |
|-------------------------|--|
| Temperature range | Can be set anywhere from 0°C to 100°C (0.1°C) |
| Temperature accuracy | Within ±2°C (set temperature and sample temperature error) |
| Temperature stability | Within ±0.5°C* |

^{*}When this product is used with a room temperature of 25°C, sample is distilled water, circulating water temperature of 22°C, and a temperature setting from 10 to 60°C. A thermostatic circulating water bath and front panel (P/N: 2J3-0182) are separately required.



Auto sipper (P/N 2J3-0131)

By pressing the front sipping lever, a sample can be drawn in from the suction nozzle and tested.

The auto sipper is suitable for multiple sample measurements.

By connecting it to an autosampler, analyses can be performed automatically, achieving labor savings.



| Minimum sample volume | 0.6 mL (when room temperature is 25 to 35°C) 0.9 mL (when room temperature is 15 to 25°C) |
|--------------------------|--|
| Wavelength range | 220 to 850 nm |
| Carry-over | 1% or less |
| Cell capacity | Approx. 50 μL |
| Sample side | 10 mm optical path length flow cell* |
| Control side | 10 mm rectangular cell can be installed |

^{*}Exchangeable with 10 mm rectangular cell holder (standard equipment). Cell is not included.

Electronic thermostatted auto sipper (P/N 2J3-0141)

This auto sipper can maintain the flow cell at a constant temperature.

| Minimum sample volume | 0.6 mL (when room temperature is 25 to 35°C) 0.9 mL (when room temperature is 15 to 25°C) |
|-------------------------|---|
| Wavelength range | 220 to 850 nm |
| Carry-over | 1% or less |
| Cell capacity | Approx. 50 μL |
| Sample side | 10 mm optical path length flow cell* |
| Set temperature | 20 to 40°C |
| Temperature accuracy | Within ±0.5°C (temperature setting and sample temperature error) When room temperature is from 15 to 25°C, sample is distilled water, and temperature setting is from 25 to 40°C. |
| Control side | 10 mm rectangular cell can be installed |

^{*}Exchangeable with 10 mm rectangular cell holder (standardequipment).

Cell is not included.

^{*}A front panel (P/N: 2J3-0182) is separately required when using this product.

^{*}Temperature control for flow cell only.

^{*}A front panel (P/N: 2J3-0182) is separately required when using this product.



Auto Sampler (P/N 2J1-0121, 2J1-0122)

In combination with an auto sipper, this unit can make multiple automatic measurements of solution samples. A suction needle can be moved in three (XYZ) directions.



| | 12 mm outer diameter, 105 mm high |
|----------------|--|
| Test tube size | 15 mm outer diameter, 105 mm high(option required) |

Film holder (P/N 210-2112)

This holder is used for measuring the transmittance and absorbance of film-like samples.



| Sample size | 25 mm wide, 30 to 50 mm high |
|---------------------|------------------------------|
| Light beam aperture | 12 mm wide, 22 mm high |

Glass filter holder (P/N 210-2109)

This holder is used for measuring the transmittance and absorbance of solid plate samples such as glass filters.



| Sample thickness | 0.5 to 5 mm |
|------------------|-----------------------|
| Sample size | 12×25 mm to 55×100 mm |

^{*}Test tube is separately required.



Polarizer holder (P/N 210-2130)

The sample beam is linearly polarized, and the polarization properties are measured. This can be used in combination with an analyzer.



| Wavelength range | 400 to 750 nm |
|------------------|-------------------------------|
| Sample thickness | 0.5 to 5 mm |
| Sample size | Min:12×25 mm / Max: 55×100 mm |

Φ60 Integrating Sphere (P/N 2J3-0176)

This is used for absorbance measurements of turbid samples and reflectance measurements of solid sample surfaces.



| Wavelength range | 220 to 2600 nm |
|---|---|
| Samples that can be installed | Transmission: Rectangular cells with 10, 20, 30, and 40 mm optical path length* Reflection: Plate specimens with sizes of Φ30 to 80 mm30×30 to 80×80 mm, and thicknesses of 10 mm or less |
| Aperture ratio | 8.1% |
| Incidence angle forreflection sample mounting position* *RS in reversed state | Sample side: 0° Control side: 8° |

^{*}For transmission, when measuring plate-shaped specimens, please order sample clamp with transmission opening (P/N: 130-2070) and cell stand (P/N: 130-2076) separately.



5° Specular Reflectance Accessory (relative) (P/N 2J3-0151)

This accessory uses the mirror reflection of a sample to measure relative reflectance with respect to a standard reflection plate (aluminum-evaporated plane mirror). This is used for film thickness measurement, spectral reflectance measurement, and other such applications.



| Incidence angle | 5° |
|---------------------------|----------------|
| Size of sample surface | 25 mm diameter |

Reference-side attenuation filter holder (P/N 2J3-0120)

This is used when you wish to expand the photometric range of the near-infrared region. To perform a measurement where you want to expand the photometric range in the near-infrared region, a NENIR210B nearinfrared absorbing ND filter, Inc. described in the table below is needed in addition to a reference-side attenuation filter holder (2J3-0120).



Must be purchased separately (customer to install)

| Product name | Manufacturer |
|---|-----------------|
| Near-infrared region absorptive ND filter NENIR210B | Thorlabs, Inc.* |

Holder set for pen-type low-pressure mercury lamp (P/N 2J3-0110)

This holder set is used when carrying out wavelength calibration or verification of wavelength accuracy using a mercury lamp. The set includes a holder to install the mercury lamp in the device and a purpose-built light source chamber cover. In addition to this product, to carry out measurements using the mercury lamp, a pen-type low-pressure mercury lamp 81-1057-98 made by BHK, Inc. and a BHK purpose-built power source 90-0005-01 are required.







Option Package Program (P/N 2J3-0191)

The UV Solutions Plus optional software is for performing calculations based on a wide variety of JIS Standard tests and various optical characteristics. By installing this program, calculations such as color calculations, direct light/solar calculations (glass), and solar reflectance paint calculations can be performed.

Main calculation features

- Color calculation
- Direct light/solar calculation (glass) JIS R 3106
- Solar reflectance paint JIS K 5602, JIS K 5675
- Film thickness calculation
- Summation
- Spectrum correction
- Thickness conversion

Main calculation features

Tristimulus value (JIS Z 8781), XYZ color space (JIS Z8781-3), L*a*b* color space (JIS Z 8781-4), Hunter Lab color space, L*u*v* color space (JIS Z 8781-5), dominant wavelength / excitation purity (JIS Z 8781-3), whiteness (JIS Z 8715), HV/C (JIS Z 8721), yellow index (JIS K 7373), change in yellowness index (JIS K 7373), color difference (L*a*b* color space (JIS Z 8781-4), Hunter Lab color space, L*u*v* color space (JIS Z 8781-5), chromaticity coordinate display



HPLC Servicing, Validation, Trainings and Preventive Maintenance:

HPLC Servicing: HPLC Servicing: We have team of service engineers who can attend to any make of HPLC promptly @the most

affordable cost.

Trainings :We also take up preventive Maintenace to reduce downtime of HPLC's Trainings.

AMC's/CMC :AMC's/CMC :We offer user training both in-House and at customer sites on HPLC principles, operations, trouble-

shooting.

Validations :Validations :We have protocols for carrying out periodic Validations as per GLP/GMP/USFDA norms.

Instruments: We offer instruments/Renting Services Modules like pumps, detector etc. on Rent.





About Analytical Technologies

Analytical Technologies is synonymous for offering technologies for doing analysis and is the Fastest Growing Global Brand having presence in at least 96 countries across the global. Analytical Technologies Limited is an ISO:9001 Certified Company engaged in Designing, Manufaturing, Marketing & providing Services for the Analytical, Chromatography, Spectroscopy, Bio Technology, Bio Medical, Clinical Diagnostics, Material Science & General Laboratory Instrumentation. Analytical Technologies, India has across the Country operations with at least 4 Regional Offices, 6 Branch Offices & Service Centers. Distributors & Channel partners worldwide.

Our Products & Technologies



UV/VIS Spectro 2080+ Double Beam



Infra FTIR



Optima Gas Chromatograph 3007



Optima Gas Chromatograph 2979 Plus



Flash Chromatograph



Atomic Absorption Spectrophotometer



Liquid Partical Counter



Optical Emission Spectrophotometer



DSC/TGA



Semi Auto Bio Chemistry Analyzer



HEMA 2062 Hematology Analyzer



Micro Plate Reader/Washer



URINOVA 2800 Urine Analyzer



Total Organic Carbon 3800



Fully Automated CLIA



NOVA-2100 Chemistry Analyzer



PCR/Gradient PCR/ RTPCR



TOC Analyzer



Laser Particle Size Analyzer



Ion Chromatograph



Water purification system

Regulatory compliances



Corporate Social Responsibility

Analytical Foundation is a nonprofit organization (NGO) found for the purpose of:



- 1.Research & Innovation Scientist's awards/QC Professional Award: Quality life is possible by innovation only and the innovation is possible by research only, hence ANALYTICAL FOUNDATION is committed to identify such personallities for their contributions across various field of Science and Technology and awarding them yearly. To participate for award, send us your details of research / testing / publication at Info@analyticalfoundation.org
- 2. Improving quality of life by offering YOGA Training courses, Work shops/Seminars etc.
- 3. ANALYTICAL FOUNDATION aims to DETOXIFY human minds, souls and body by means of yoga, Meditation, Ayurveda, Health Care, Awards, Media, Events, Camps etc.





HPLC Solutions MultipleLabs Analytical Bio-Med Analytical Distributors Analytical Foundation (Trust)